### **Specifications**

Microscope unit

Microscope unit		
Туре		Galileo type
Magnification		Drum, 5-step magnification
Magnification steps		6/10/16/25/40
Overall magnification (actual vision field)		6.37 (φ 35.1mm)
		9.94 ( $\phi$ 22.5mm)
		15.87 (φ14.1mm)
		25.37 (\$\$ 8.8mm)
		39.62 (\$ 5.6mm)
Eyepiece lens	Magnification	12.5x
	Diopter adjustment range	-5D to +5D
Binocular tubes		PD adjustment: 55 to 78mm
Illumination unit		
Illumination field	Slit width	0 to 14mm, adjustable (14mm=circle)
indimination neid	Slit length	14mm to 1mm, adjustable (14mm=circle)
	Aperture diameter	
Slit direction	Aperture diameter	φ 14, 10, 5, 2, 1, 0.2 mm
		Vertical to horizontal, adjustable
		Inclination: 5°/10°/15°/20 °
		Side swing
Filter		Blue filter, red-free filter, amber filter,
		UV cut filter (normal use)
		ND filter (13% transmission)
Illumination lamp	LED type	3A, 10W
Base unit		
Forward-backward movement		90mm
Right-left movement		100mm
Vertical movement		30mm
Amount of movement in all directions		12mm
Chinrest unit		
Amount of vertical movement of chinrest		80mm
Fixation target		Fixation target with diopter adjustment
		Luminous fixation target
Fixation lamp		LED (Red)
Other Specification	าร	
Dimensions	w/Table	550mm(W) x 420mm(D) x 752 to 782mm(H)
	w/ Unit Table	440mm(W) x 397mm(D) x 752 to 782mm(H)
	w/o Table	329mm(W) x 396mm(D) x 652 to 682mm(H)
	w/o Table and Chinrest	329mm(W) x 331(304)mm(D) x 652 to 682mm(H)
	Weight: w/Table	19kg
	w/ Unit Table	18kg
	w/o Table	13kg
	w/o Table and Chinrest	11.5kg
	Table size	550mm x 370mm
	Unit Table size	440mm x 350mm
	Height from the top to patient's eye	375mm
Power Supply		100-240V AC, 50-60Hz, 110VA

Power Supply

CE

\*Subject to change in design and/or specifications without advanced notice.

IMPORTANT In order to obtain the best results with this instrument, please be sure to review all user instructions prior to operation.

#### PERFORMANCE YOU CAN COUNT ON ΤΟΡΟΟΛ

TOPCON MEDICAL LASER SYSTEMS, INC.

3130 Coronado Drive Santa Clara California 95054 USA Phone:+1-408-235-8200 Phone:(USA only)+1-888-760-8657 Fax:+1-408-235-8259 Email: tmlsinfo@topcon.com

Pat:+1-408-239-2539 Entail Institute report com **TOPCON CANADA** Institute report com 110 Provencher Avenue, Boisbriand, QC J7G 1N1 CANADA Phone:+1-450-430-7771 Fax:+1-450-430-6457 www.topcon.ca

E-mail: medical@topcon.nl; www.topcon.eu ITALY OFFICE Viale dell'Industria 60: 20037 Paderno Dugnano; (Milano), ITALY Phone:+39-02-9186671 Fax:+39-02-91081091 E-mail: topconitaly@tiscali.it; www.topcon.it

TOPCON EUROPE MEDICAL B.V.

CPCUN EUROPE INERIONE INCLORED AND A CONTRACT AND A

DANMARK OFFICE Praestemarksvej 25: 4000 Roskilde, DANMARK Phone:+45-46-327500 Fax:+45-46-327555 E-mail: topcon@topcondanmark.dk www.topconda

#### TOPCON CORPORATION ii-ku, Tokyo 174-8580, Japan. Phone:3-3558-2523/2522 Fax:3-3965-6898 www.topcon.co.jp

TOPCON MEDICAL SYSTEMS, INC.

- TOPCON S.A.R.L. BAT A1 3 route de la révolte 93206 SAINT DENIS CEDEX Tel : +33 1 49 21 23 23 Fax : +33 1 49 21 23 24 E-mail.top 1 49 21 23 24 E-mail:topc opcon.fr; www.topcon.f TOPCON DEUTSCHLAND G.m.b.H. Hanns-Martin-Schleyer Strasse 41; D-47877 Willich, G Phone:+49-10/2154-8850 Fax:+49-(0)/2154-885177 E-m
  - TOPCON SCANDINAVIA A.B.

TOPCON ESPAÑA S.A.

HEAD OFFICE Frederic Mompou 4 Esc. A Bajos 3, 08960 Sant Just Desvern Barcelona, SPAIN Phone:+34-93-4734057 Fax:+34-93-4733932 E-mail: medica@topcon.es; www.top

- TOPCON ( GREAT BRITAIN ) LTD. hire RG14 5PX United Kir 85-551120 Fax:+44-(0)1635-551170 E-mail:
- TOPCON POLSKA Sp. z. o. o. ul. Warszawska 23; 42-470 Siewierz, POLAN Phone:+48-(0)32-6705045 Fax:+48-(0)32-67

TOPCON SINGAPORE MEDICAL PTE. LTD. 1 JALAN KILANG TIMOR #09-01 PACIFIC TECH CENTRE SINGAPORE 159303 Phone:+65-68720606 Fax:+65-67736150 E-mailmedicaLsales@topcon.com.sg www.topcon.co

#### TOPCON INSTRUMENTS ( MALAYSIA ) SDN.BHD.

ISO 14001

JAC())

EC97J1081

o. D1, (Ground Floor), Jalan Excella 2, Off Jalan Amp iman Ampang Hilir, 55100 Kuala Lumpur, MALAYSIA 10ne:+60-(0)3-42709866 Fax:+60-(0)3-42709766 TOPCON INSTRUMENTS ( THAILAND ) CO., LTD.

Klongsarn, Bangkok 10600, THAILA TOPCON CORPORATION BEIJING OFFICE

TOPCON CORPORATION SHANGHAI OFFICE


- 14L Huamin Empire Plaza, No.726, Yan-an Xi Road, Shanghai, 200050, CHINA Phone: +86-(0)21-5238-7722 Fax:+86-(0)21-5237-076
- TOPCON CORPORATION BEIRUT OFFICE P.O.Box 70-1002 Antelias,Beirut, LEBANON
- TOPCON CORPORATION DUBAI OFFICE

О,

SGS

TOPCON CORPORATION TOPCON CORPORATION TOPCON CORPORATION

P.O.Box 293705, Dubai Airport Free Zone L.I.U. J-12, Dubai, U.A.E Phone:+971-4-299-5900 Fax:+971-4-299-5901

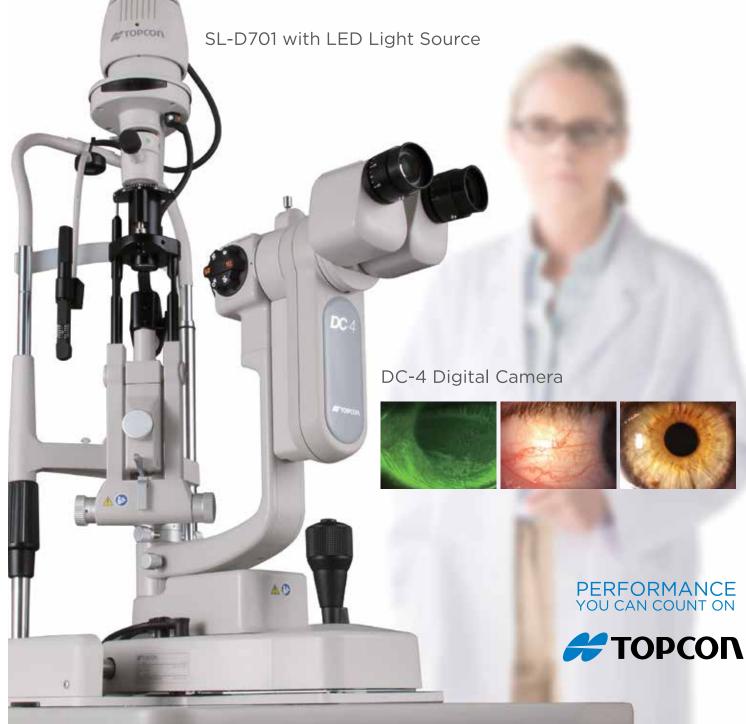

## **SL-D701** Digital Slit Lamp




### **Features**

- » LED Illumination Source
- » Apochromatic Optics with Protective Coating
- » Selectable Amber Filter for Color Correction
- » Five Magnifications Selectable by Rotating Drum

### **Optional DC-4 Digital Camera**

- » High Resolution
- » Smart Capture Function
- » Video Capability
- » Auto Exposure

### Advantages and Benefits of LED

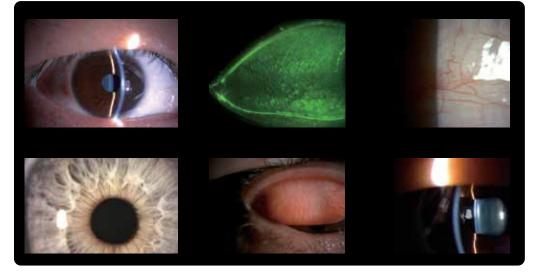

### **LED Illumination Source**

The new LED illumination source allows observation under a brighter and more homogeneous light condition compared to the conventional halogen bulb source. Color temperature remains uniform when adjusting light intensity insuring consistent viewing results. The short wavelength of the LED spectrum allows for the observation of minute details.

### Advantages of LED Illumination

- » Brighter illumination enhances observation of the eye structures
- » Wavelength characteristics allow for easy visualization of subtle details
- » Consistent color temperature throughout the entire intensity adjustment
- » Substantial reduction in bulb replacement
- » Energy and cost savings

### Meibomian Gland Observation


Meibomian gland observation and documentation is possible when using the optional DC-4, BG-5 digital photo attachment and background illuminator.

#### **Different Conditions of Meibomian Glands**




**Meibomian Gland Close-up** 





Images courtesy of Reiko Arita, MD, PhD. Itoh Clinic, Department of Ophthalmology, University of Tokyo School of Medicine

### System Chart

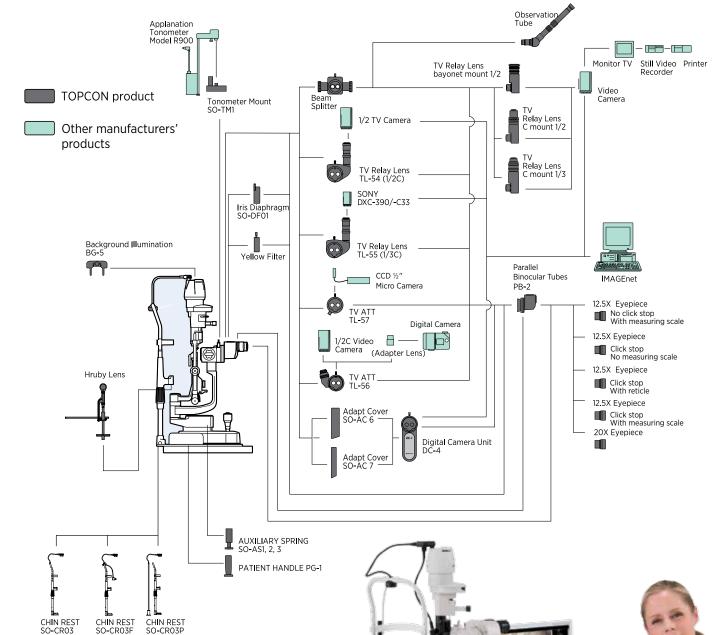

# SL-D701 with LED Light Source

Shown with optional DC-4 Digital Attachment and BG-5 Background Illuminator, optional handle bars and optional instrument table. NOTE: Optional instrument table not available in all markets.

